


DIABETIC FOOT SCREEN FOR LOSS OF PROTECTIVE SENSATION

National Hansen's Disease Programs, LEAP Program, 1770 Physicians Park Dr., Baton Rouge, LA 70816




Filament Application Instructions:

- 1) Show the filament to the patient and touch it to his/her hand or arm so that he/she knows it does not hurt.
- 2) Use the 10 gram filament to test sensation at the indicated sites on each foot as shown. Apply the filament along the perimeter of and NOT on an ulcer, callous, scar, or necrotic tissue.

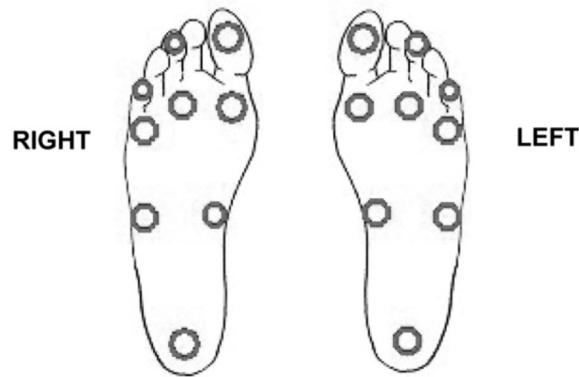

Note: While five sites on each foot are necessary for proper sensation testing, additional sites are preferred, as shown here.

- 3) Hold the filament perpendicular to the skin and use a smooth motion when testing. Use a 3 step sequence that includes (1) touch the skin, (2) bend the filament, and (3) lift from the skin (*See Figures 1-3*). Do not use rapid movement. The approach, skin contact, and departure of the filament should be approximately 1½ seconds duration.



- 4) Ask the patient to respond "yes" when the filament is felt. If the patient does not respond when you touch a given point on the foot, continue on to another site. When you have completed the sequence, REPEAT the area(s) where the patient did not indicate feeling the filament.
- 5) Use the filament in a random sequence.
- 6) On the form, indicate with a minus sign, "—", the areas where the patient did not respond to the filament. LOSS OF PROTECTIVE SENSATION AT ANY ONE OF THE EIGHT SITES INDICATES A FOOT AT HIGH RISK.
- 7) If you wish to clean the filament, use sodium hypochlorite (*household bleach*) 1:10 solution or follow the infection control disinfecting guidelines in your facility.

JF/06/2005